


Percutaneous Endoscopic Gastrostomy Kit

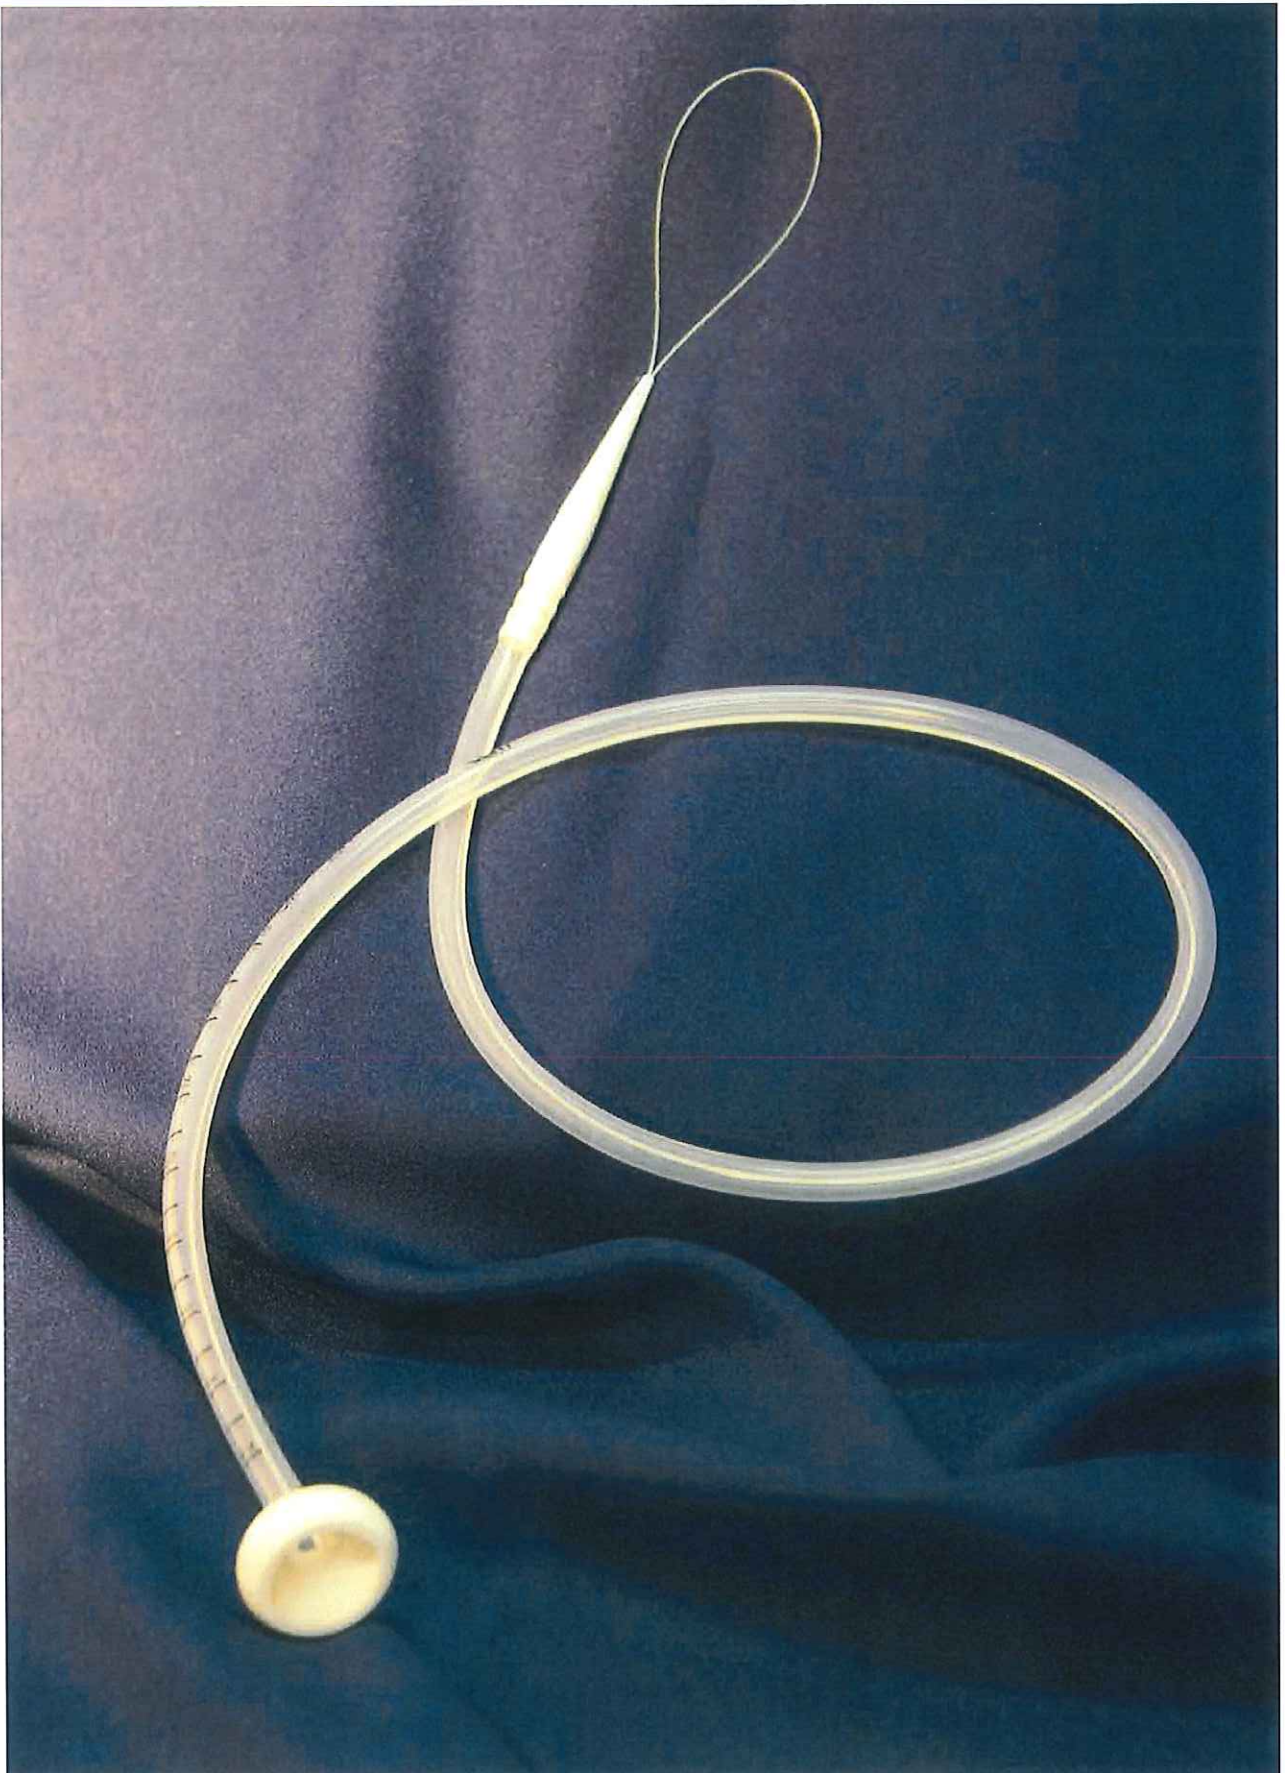

For the safety initial PEG placement procedure

Initial Placement Kit

1. Standard Kit

Product Number	Size	Placement Method	Package	Sterilization
800 001 4916	20Fr	Pull Type	1Kit	EtO Gas
800 001 4917	24Fr	Pull Type	1Kit	EtO Gas

Contents:


- | | |
|-----------------|------------------------------|
| ①PEG catheter | ⑤Introducer Needle |
| ②2 port adaptor | ⑥Stabilizer (Retention ring) |
| ③Scalpel | ⑦Loop wire |
| ④Clamp | |

2. Full Kit

Product Number	Size	Placement Method	Package	Sterilization
800 001 4914	20Fr	Pull Type	1Kit	EtO Gas
800 001 4915	24Fr	Pull Type	1Kit	EtO Gas

Contents:

- | | | |
|------------------------------|-------------|--------------------|
| ①PEG catheter | ⑦Loop wire | ⑬Sponge with grip |
| ②2 port adaptor | ⑧Snare | ⑭Hemostat |
| ③Scalpel | ⑨Drape | ⑮Scissors |
| ④Clamp | ⑩Syringe | ⑯Needles (19G&25G) |
| ⑤Introducer Needle | ⑪Bite block | ⑰Gauze |
| ⑥Stabilizer (Retention ring) | ⑫Prep razor | |

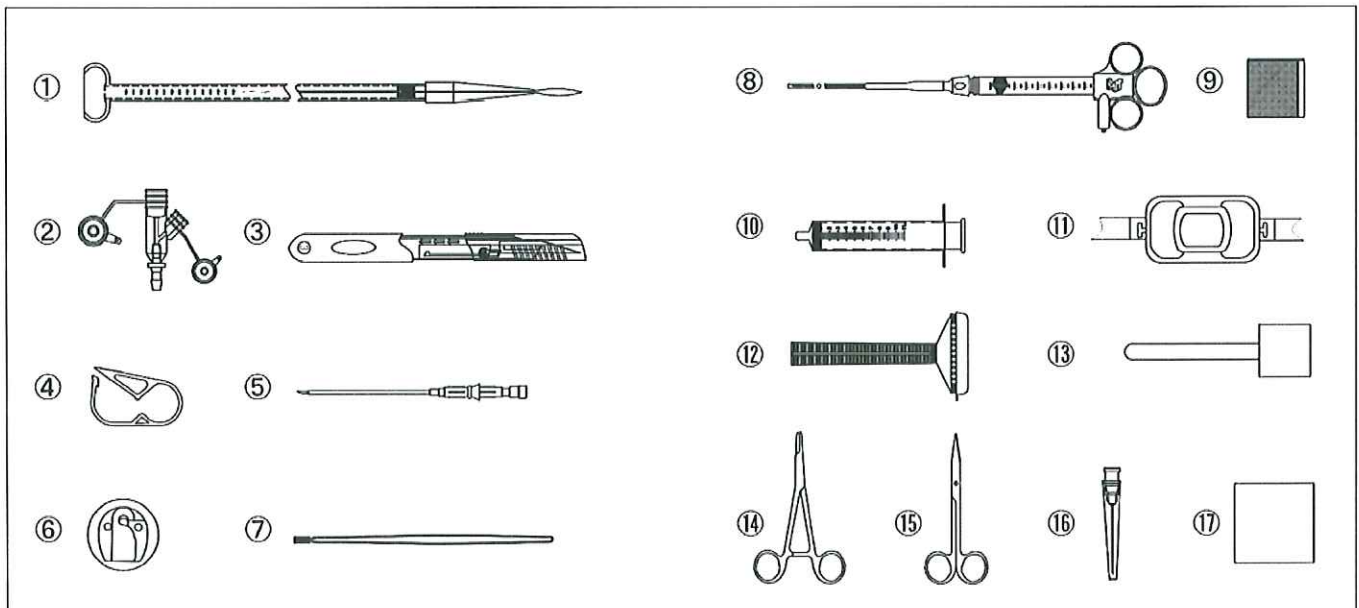

- Please note that a partial amendment in specifications is made occasionally, as studies and developments have been performed continuously.
- Be sure to read through the instructions for use attached to the device before use.

G-017



CREATE MEDIC CO.,LTD.

Head Office

5-25 Chigasakiminami, 2-Chome, Tsuzuki-Ku, Yokohama 224-0037, Japan

Tel: +81 45-943-2741 Fax: +81 45-943-2746

E-mail: exportsales@createmedic.co.jp URL: <http://www.createmedic.co.jp>